INSTRUCTIONS FOR USE

Sure-Check® Sterilization Pouch

Available in 14 Sizes!

Instructions for use:

1. **Storage** - Store all sterilization pouches in a cool, dry place.

2. **Loading*** - Carefully place items into pouches and remove excess air before sealing. Where possible, use a pouch rack to stand pouches on edge in the sterilizer to facilitate sterilization and drying. When loading multiple pouches, be sure that the plastic side faces the paper side of each adjacent pouch.

3. **Sterilization** - Steam chemical indicator ink printed on the inside of each Sure-Check® pouch is certified as a multi-variable (parameter) indicator. Internal multi-variable (parameter) chemical indicators are designed to react to the 3 variables required for sterilization - temperature, specified time, presence of steam - and provide a more reliable indication that the conditions for sterilization have been met. Pink indicators will turn brown when processed by steam. Blue indicators will turn gold/brown when EtO processed. Multi-variable (parameter) indicators meet the 2008 CDC †Guidelines for sterilization. Sure-Check® pouches are only available for use in steam sterilizers (autoclaves) and EtO. This procedure, when used in conjunction with routine biological monitoring (spore testing), provides you with the highest level of sterility assurance.

Ref.#'s SCXX2, SCX2, SCXS2, SCS2, SCS25, SCL3222, SCW2, SCM2, SCL5152, SCL2, SCL8162, SCL10152, SCL10172, SCL12152, SCL12182

4. **Shelf Life** - When properly sealed, sterility is maintained up to three (3) years provided the integrity of the pouch has not been compromised, i.e. pouch becomes wet, damaged or is opened during storage.
Caution - wet pouches may not preserve sterility of contents.

Sure-Check sterilization pouches are single use items. Do not re-use.

Sure-Check® Sterilization Pouches are not considered hazardous waste and can be disposed of in regular trash (40 CRF 261.24 tested using the TCLP, EPA Publication SW-846).
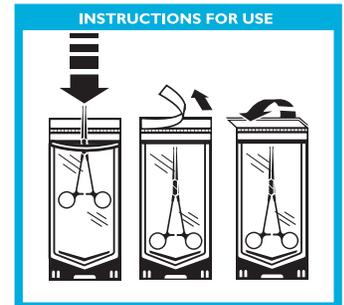
INSTRUCTIONS FOR USE

* REFERENCE - ANSI/AAMI ST79 Comprehensive Guide to Steam Sterilization and Assurance in Health Care Facilities.
† CDC Guideline for Disinfection and Sterilization in Healthcare Facilities, 2008.

Sure-Check® is a registered trademark of Crosstex International, Inc.

Do not reuse.

LATEX

Not made with natural rubber latex.

CROSSTEX®
A CANTEL MEDICAL COMPANY

Manufactured by: Crosstex International, Inc.
10 Ranick Road | Hauppauge, NY 11788 | 631.582.6777 | 888.276.7783 | Crosstex@crosstex.com

| EC | REP | MDSS GmbH Schiffgraben 41 30175 Hannover, Germany |

CE

Made in USA