



Accutron™ Axess™ Capnography Adapter INSTRUCTIONS

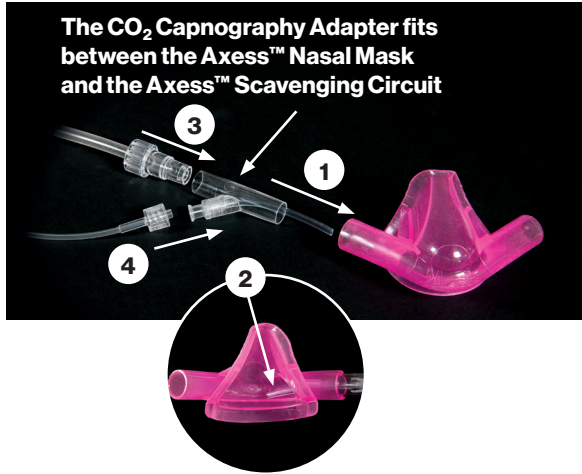

- 1 Install the Capnography Adapter into the Axess Mask (*adapter can be inserted on either side of the mask*).
- 2 **NOTE:** The end of the Capnography Extension Tube should be visible inside the Axess Nasal Mask.
- 3 Insert the Mixed Gas Fitting (*stepped-shaped fitting*) into the Capnography Adapter.
- 4 Twist/attach the sampling line from the Capnography Monitor to the Luer-Lok® Fitting on the Capnography Adapter.
- 5 Discard the CO₂ Capnography Adapter along with the Mask at the end of the procedure.
NOTE: Single-Use Only

NOTE: Capnography Monitoring is the monitoring of carbon dioxide exhaled by the patient. It is sometimes referred to as CO₂ monitoring or ETCO₂ monitoring.


Accutron™ Axess™ Capnography Adapter INSTRUCTIONS

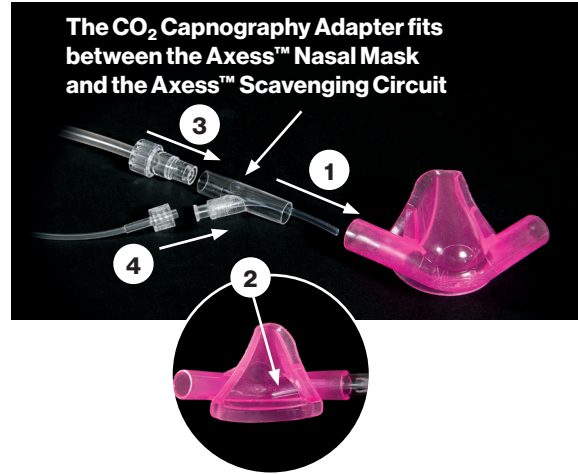

- 1 Install the Capnography Adapter into the Axess Mask (*adapter can be inserted on either side of the mask*).
- 2 **NOTE:** The end of the Capnography Extension Tube should be visible inside the Axess Nasal Mask.
- 3 Insert the Mixed Gas Fitting (*stepped-shaped fitting*) into the Capnography Adapter.
- 4 Twist/attach the sampling line from the Capnography Monitor to the Luer-Lok® Fitting on the Capnography Adapter.
- 5 Discard the CO₂ Capnography Adapter along with the Mask at the end of the procedure.
NOTE: Single-Use Only

NOTE: Capnography Monitoring is the monitoring of carbon dioxide exhaled by the patient. It is sometimes referred to as CO₂ monitoring or ETCO₂ monitoring.

Accutron™ Axess™ Capnography Adapter INSTRUCTIONS

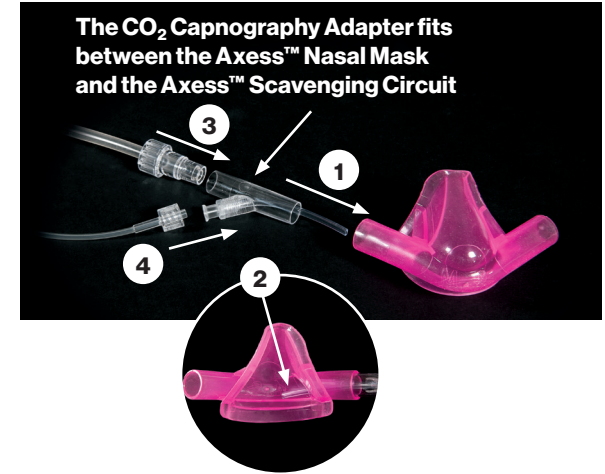

- 1 Install the Capnography Adapter into the Axess Mask (*adapter can be inserted on either side of the mask*).
- 2 **NOTE:** The end of the Capnography Extension Tube should be visible inside the Axess Nasal Mask.
- 3 Insert the Mixed Gas Fitting (*stepped-shaped fitting*) into the Capnography Adapter.
- 4 Twist/attach the sampling line from the Capnography Monitor to the Luer-Lok® Fitting on the Capnography Adapter.
- 5 Discard the CO₂ Capnography Adapter along with the Mask at the end of the procedure.
NOTE: Single-Use Only

NOTE: Capnography Monitoring is the monitoring of carbon dioxide exhaled by the patient. It is sometimes referred to as CO₂ monitoring or ETCO₂ monitoring.



Accutron, Inc.
1625 W. Pinnacle Peak Rd., Phoenix, AZ 85027 USA
800.531.2221 | HuFriedyGroup.com/Accutron

EU **REP** MT Promedt Consulting GmbH
Ernst-Heckel-Straße 7
66386 St. Ingbert
Germany

CH **REP** MDSS CH GmbH
Laurenzenvorstadt 61
5000 Aarau
Switzerland

UK **REP** MDSS-UK RP Ltd.
6 Wilmslow Road, Rusholme
Manchester M14 5TP
United Kingdom



0482

US Made in USA
28598 / REV 2 - 08/2025

All company and product names are trademarks of Hu-Friedy Mfg. Co., LLC, its affiliates or related companies, unless otherwise noted.

Luer-Lok® is a registered trademark of Becton Dickinson and Company.

©2025 Hu-Friedy Mfg. Co., LLC. All rights reserved.



Accutron, Inc.
1625 W. Pinnacle Peak Rd., Phoenix, AZ 85027 USA
800.531.2221 | HuFriedyGroup.com/Accutron

EU **REP** MT Promedt Consulting GmbH
Ernst-Heckel-Straße 7
66386 St. Ingbert
Germany

CH **REP** MDSS CH GmbH
Laurenzenvorstadt 61
5000 Aarau
Switzerland

UK **REP** MDSS-UK RP Ltd.
6 Wilmslow Road, Rusholme
Manchester M14 5TP
United Kingdom



0482

US Made in USA
28598 / REV 2 - 08/2025

All company and product names are trademarks of Hu-Friedy Mfg. Co., LLC, its affiliates or related companies, unless otherwise noted.

Luer-Lok® is a registered trademark of Becton Dickinson and Company.

©2025 Hu-Friedy Mfg. Co., LLC. All rights reserved.



Accutron, Inc.
1625 W. Pinnacle Peak Rd., Phoenix, AZ 85027 USA
800.531.2221 | HuFriedyGroup.com/Accutron

EU **REP** MT Promedt Consulting GmbH
Ernst-Heckel-Straße 7
66386 St. Ingbert
Germany

CH **REP** MDSS CH GmbH
Laurenzenvorstadt 61
5000 Aarau
Switzerland

UK **REP** MDSS-UK RP Ltd.
6 Wilmslow Road, Rusholme
Manchester M14 5TP
United Kingdom



0482

US Made in USA
28598 / REV 2 - 08/2025

All company and product names are trademarks of Hu-Friedy Mfg. Co., LLC, its affiliates or related companies, unless otherwise noted.

Luer-Lok® is a registered trademark of Becton Dickinson and Company.

©2025 Hu-Friedy Mfg. Co., LLC. All rights reserved.